PCB Piezotronics Inc. claims proprietary rights in the information disclosed hereon. Neither it nor any reproduction thereof will be disclosed to others without the written consent of PCB Piezotronics Inc.

11681

REVISIONS

REV	DESCRIPTION	DIN
B	ADDED ±.001 TO Ø.101 AND Ø.156, UPDATED TITLE BLOCK, & Ø.247 ±.001 WAS Ø.248 +.000/-.002	50148

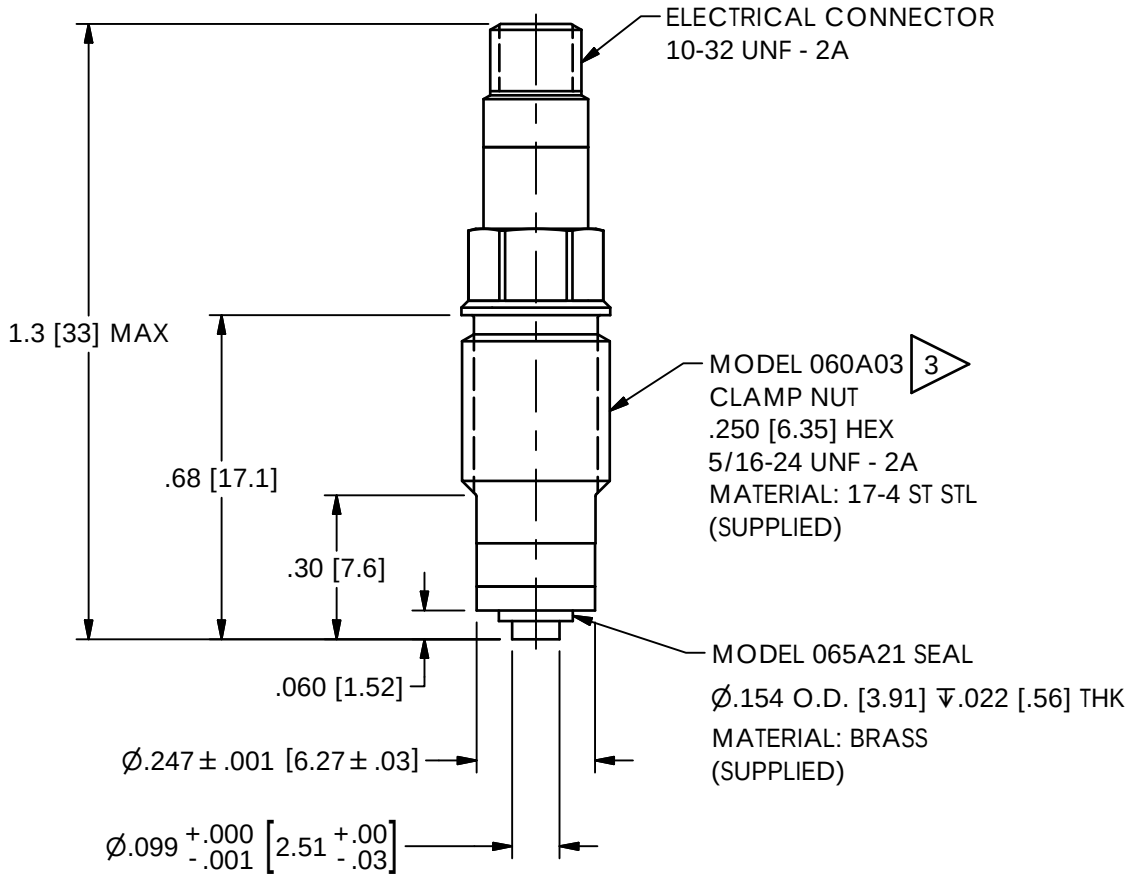

MOUNTING HOLE PREPARATION:

Ø.101± .001 [2.60± .03] THRU 1

⌴Ø.156± .001 [4.00± .03] ↧.605 +.001 -.005 [15.38 +.03 -.13] 1

⌴Ø.250 +.005 -.000 [6.40 +.13 -.00] ↧.590 +.000 -.002 [14.99 +.00 -.05] 1

Ø.272 [6.90] ↧.465 [11.81]

5/16-24 UNF - 2B ↧.350 [8.89]

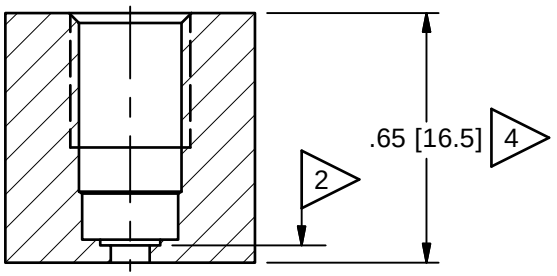

4 FOR INSTALLATIONS DEEPER THAN .65 [16.5], ⌴Ø.437 [11.10] TO CLEAR .250 [6.35] HEX

3 RECOMMENDED MOUNTING TORQUE ON .250 [6.35] HEX: 2 ft lbs [2.7 Nm]

2 SEAL SURFACE MUST BE FLAT AND FREE OF TOOL MARKS

1 THESE DIAMETERS MUST BE CONCENTRIC TO WITHIN .001 [.03] TIR

UNLESS OTHERWISE SPECIFIED TOLERANCES ARE:		DRAWN		CHECKED		ENGINEER	
DIMENSIONS IN INCHES	DIMENSIONS IN MILLIMETERS [IN BRACKETS]	JES	12/11/19	JES	12/11/19	MJK	12/11/19
DECIMALS XX ±.01 XXX ±.005	DECIMALS X ± 0.3 XX ± 0.13	TITLE					
ANGLES ± 2 DEGREES	ANGLES ± 2 DEGREES	INSTALLATION DRAWING MODEL 105CX3 SERIES PRESSURE SENSOR					
FILLETS AND RADII .003 - .005	FILLETS AND RADII 0.07 - 0.13						

PCB PIEZOTRONICS
3425 WALDEN AVE. DEPEW, NY 14043
(716) 684-0001 E-MAIL: sales@pcb.com

CODE IDENT. NO.	DWG. NO.	
52681	11681	
SCALE: 2.5X	SHEET 1 OF 1	